

# **15 High Touch Surfaces**

## **Public Areas**

1. Public café table
2. Public break room table
3. Public bathroom door handle (inside)
4. Public bathroom faucet handle
5. Public information desk
6. Blood pressure cuff


## **Patient Room**

1. Bedside table handle
2. Call box/button
3. Bedrails/bed controls
4. Door handle inside room

## **Patient Bathroom**

1. Toilet seat
2. Toilet flush handle
3. Bathroom light switch
4. Bathroom door knob outside
5. Bathroom hand rails

# ATP Testing Procedure

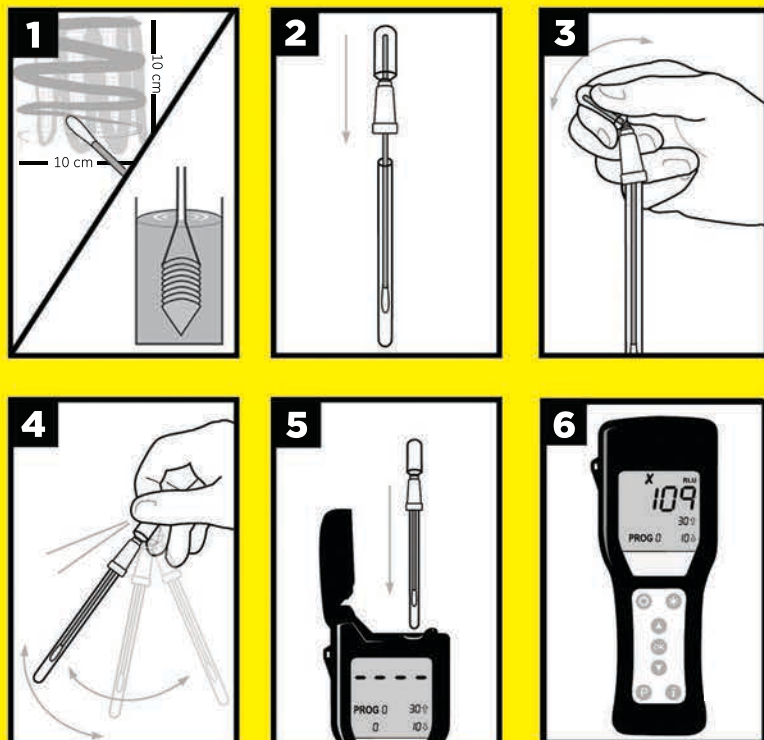

Turn on luminometer and wait 15 seconds for calibration check.  
Select user and test location. (See reverse for instructions).

1. Remove swab from test tube and collect sample. Refer to instructions included with the testing device or watch an instructional demo at [www.youtube.com/HygienaTV](http://www.youtube.com/HygienaTV)
2. Place swab back in test tube.
3. Snap bulb by bending back and forth and squeezing to expel liquid reagent into swab tube.
4. Lightly shake for 5 seconds, bathing swab in liquid.
5. Place swab test in luminometer and close lid.
6. Press "OK" and reading will appear in 15 seconds.



## Helpful Tips Hygiena Monitoring System




1. When taking sample readings, be sure to hold the luminometer upright.
2. Do not overload test swabs. Collecting samples from visibly contaminated surfaces could inhibit reaction. Do not test a surface that is visibly dirty.
3. Before using AquaSnap test devices, flick test in a downward motion to bring extractant liquid into bottom of tube.
4. If the instrument will not calibrate, be sure the lid is completely closed by tucking the rubber flap over the data port underneath the plastic edge.
5. Do not allow any material or liquids into the test chamber of the luminometer. Always close the lid when not in use. Ensure outside of the test device is dry before inserting tests for reading.
6. Once activated, swab tests must be read immediately. Refer to individual product instructions for more details.
7. If the luminometer is moved to different areas with  $\pm 5^{\circ}\text{C}$  (  $\pm 10^{\circ}\text{F}$ ) or greater varying temperature, a temperature calibration should be performed in each new climate. Hold down "OK" button for 3 seconds to start a 15 second temperature calibration.

8. Watch instructional videos for all Hygiena products at [www.youtube.com/HygienaTV](http://www.youtube.com/HygienaTV)



1. Press the red power button to turn on the unit. Let it run through the 15 second calibration check.

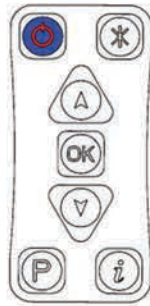



2. Once calibrated, press the “\*” button to access the menu. The first menu item is “USER ID”. Press OK to select.

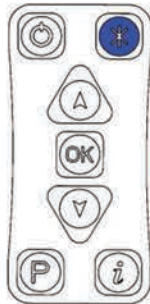


3. The User ID number will begin to flash. Use the up or down arrows to select the appropriate User ID. Press “OK” to select. The User number will stop flashing.

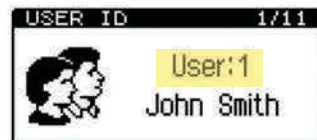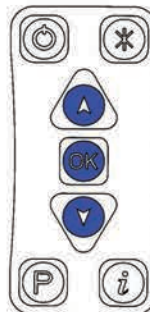



4. Press the up arrow to move to the second menu option, “TEST PLAN”, and press “OK” to select.

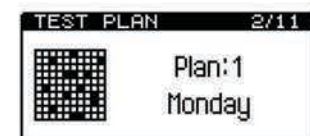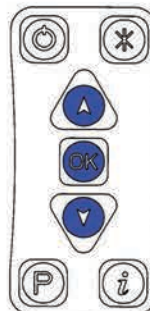


5. The Test Plan number will begin to flash. Use the up or down arrows to select the desired test plan. Press “OK” to select. The Plan number will stop flashing.

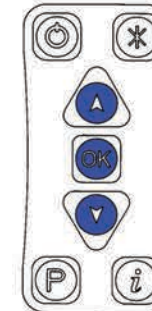



6. Press the “\*” button to return to the home screen. Test device may now be inserted for measurement.

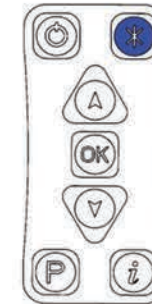

7. To move to the next test in the test plan, press “P” button. The Program number, “Prog: #”, will begin to flash.



8. Press the up arrow to move to the next test location in the plan and press “OK” to select. The Program number will stop flashing. Test device may now be inserted for measurement.

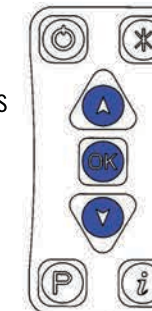

# Upper Cumberland CMP Reinvestment Program

## Sign-in Sheet

Your Name	Organization	Title/Position	Email
Heather M. Smith	<del>W</del> Wharton/Upland Village	Charge Nurse/Infection Control	<del>heather.smith</del> minman@uplandsvillage.com
Debbie Jo Gilman	Cookeville NHC	EVS Director	debbie.gilman@nhccare.com
Dawn Johnson	Life Care	RN ADON	Dawn-Johnson@LCCA.com
Christie Bond	Overton Co.	RN, IP	cbondchr@gmail.com
NATHANAEL RICH	Standing Stone Care & Rehab	RN, DON	don.standingstone@shcc.com
Brenda Jones	Signature Health Care of Fentress	Formulary/Infection Control	APN.@signaturehealthllc.com
John Wright-Blakeley	Overton County Health & Rehab	Environmental Services Director	JwrightocNH@gmail.com
Amanda Myers	Baintree Manor	QA/Infection Control	rtgan@gracehc.com
Latessa Morris	Life Care Center of Sparta	Executive Director	latessa-morris@lcca.com
Denny Bray	Life Care Center of Sparta	Director Maint Environ	Denny-bray@LCCA.com
Holly McKinnon	Generations Center of Spencer	Infection Preventionist	hsullivan@generationsquarter.com
Tammy Fox	GCO S	QA	tfox@generationsquarter.com
Daniel Mayse	NHC Cookeville	House Supervisor	Daniel.mayse@NHCCare.com
Sue Holliman	The Palace Care & Rehab	NE	PMH@NanyandHolliman-RC.com
Doris Powers	The Palace Care & Rehab	NK/Laundry Supervisor	
Amanda Wood, RN	Celina Health & Rehab	Adon	ccadon@twinrivershc.com
Cassey Malone	Standing Stone Care & Rehab	Administrator	admin.standingstone@shccs.com
Ruthie Bindwell	SHC Putnam	DON	DON.Cookeville@shccs LLC.com



# Upper Cumberland CMP Reinvestment Program

## Sign-in Sheet

Your Name	Organization	Title/Position	Email
Kim Stafford	SHC Putnam	ADON	adon2.cookeville@shccs.com
CINDY TILTON	NHC HealthCare McMinnville	RN/DON	CINDY.TILTON@NHCCARE.COM
Chrystal Parrott	Pickett Care & Rehab	RN/DON	don.pickett@shccs.com
Amy Lee	Pickett Care & Rehab	CEO	admin.pickett@shccs.com
Karen Smith	Smith County Health & Rehab	RN/DON	KSmith@Smithcountyhealthandrehab.com
Lisa Carter	Cumberland Medical Center	RN/IP	lcarter@cmchealthcare.org
Jessica Boregas	Good Samaritan	RN/IP	jboregas@good-sam.com
Kim Kuthey	Wyndridge	RN/ADON	kimk@wyndhs.com
JJ McBee	NHC Sparta	EVS Director	joyce.mcbee@nhccare.com
Brennan Pearson	NHC Sparta	Administrator	brennan.pearson@nhccare.com
Tammy Thrasher	LRH	ID, Eth, WIC	tammy.thrasher@iput.net
Brittany Lee	Knollwood Manor	DON	blee@netc.com
Leanne Bilbrey	macon Comm Hosp	DON / IPRI	
Heather Stafford	Mabry Health Care	DON	mabry.mds@gmail.com
Hope Combs	Mabry Health Care	ADON	mabry.adon@gmail.com
Nanci Drennan	NHC Smithville	LPN / IP	nanci.drennan@nhcsmithville.com